SUBJECT: Installation schematic for Isco-Stip PBS1 Ammonia Process Buoy

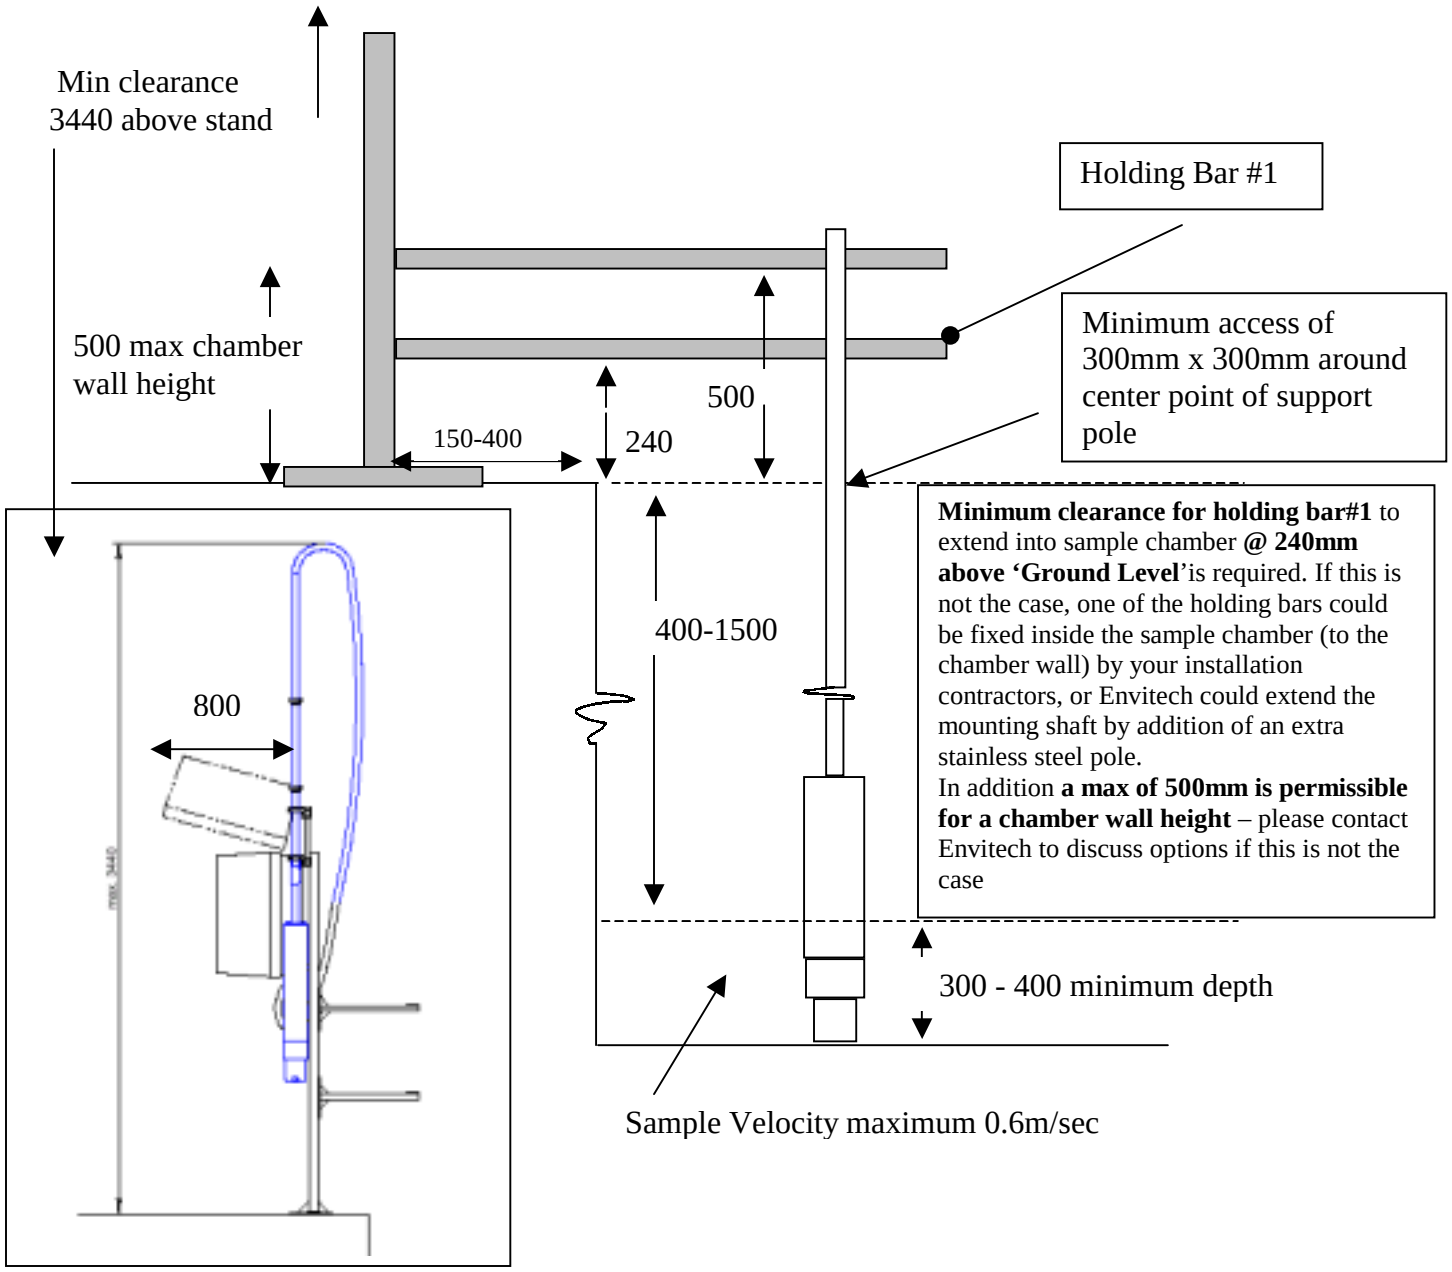

Minimum clearance for holding bar#1 to extend into sample chamber **@ 240mm above 'Ground Level'**is required. If this is not the case, one of the holding bars could be fixed inside the sample chamber (to the chamber wall) by your installation contractors, or Envitech could extend the mounting shaft by addition of an extra stainless steel pole.
In addition **a max of 500mm is permissible for a chamber wall height** – please contact Envitech to discuss options if this is not the case